



CUSTOMER:	P/N:0310.120	REV.	APPROVALED BY:	REVISIONS		
				REV.	DESCRIPTION	DATE
				A		2021.12.04
				B	Change the wire printing and winding method, change the plug to the terminal frame type	2022.07.27

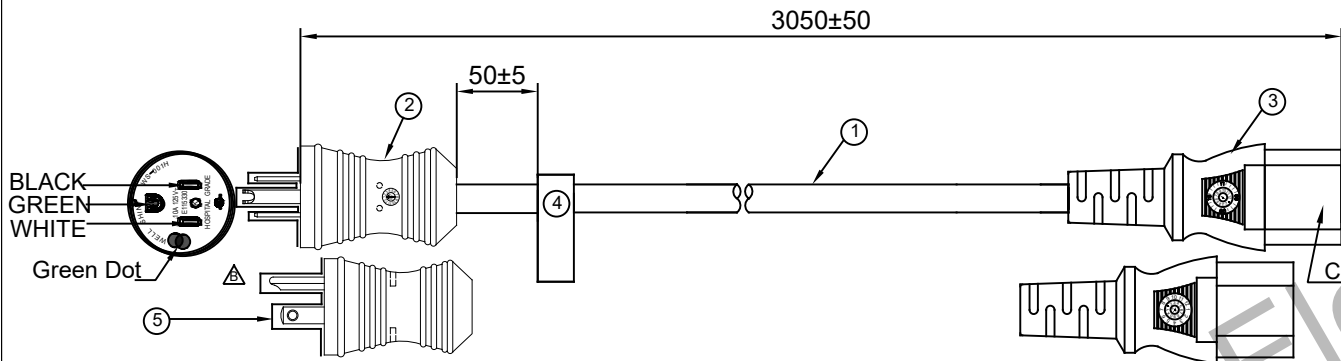


NOTES:

1. The outer box must have the RoHS mark (RoHS shown on the carton)
2. The tail WS-002 uses a transparent inner sleeve
3. The label is black on a white background, and the flag is pasted.




MARKING:




NEMA 5-15P
HOSPITAL GRADE
CLEAR


MARKING:



IEC-60320-C13
CLEAR

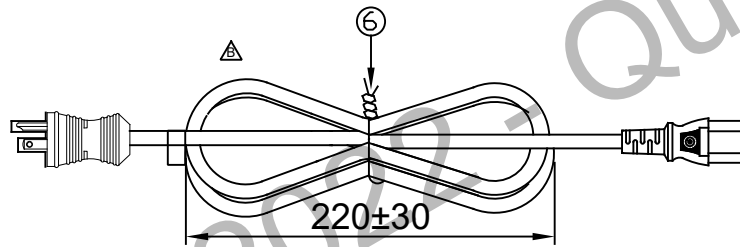

④ Hosp.Grade label

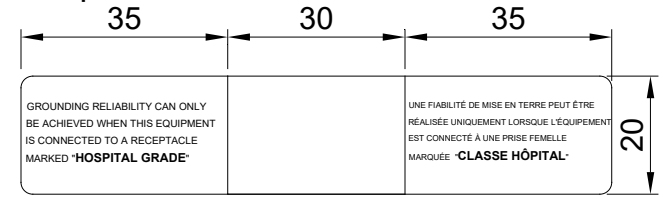

⑥	Cable tie	WHITE	1PCS
⑤	Protective case	WHITE	1PCS
④	Wire label 100mm*20mm		1PCS
③	WS-002 10A 125V APPROVAL: UL,CUL	CLEAR	1PCS
②	WS-001H(5-15P) 10(A) 125(V) APPROVAL: UL,CUL	CLEAR	1PCS
①	C(UL)US E90165-K SJTW 3×0.824mm ² (18AWG) with thread 105°C 300V VW-1 WELL SHIN	GRAY	1PCS
NO.	DESCRIPTION	COLOR	QTY

SIGNATURE		QUAIL ELECTRONICS, INC.® http://www.quail.com	
ENGINEER BY:		PRODUCT NO.WS-001H-1+002-1	DATE: 2021.11.22
MANAGER BY:		UNIT: mm	SHEET:1 OF 11
CHECKED BY:		DWG NO:0096-8351	
DRAWN BY:		B	